


Cole-Parmer®

WD-200 Series

Paraffin Wax Dispenser

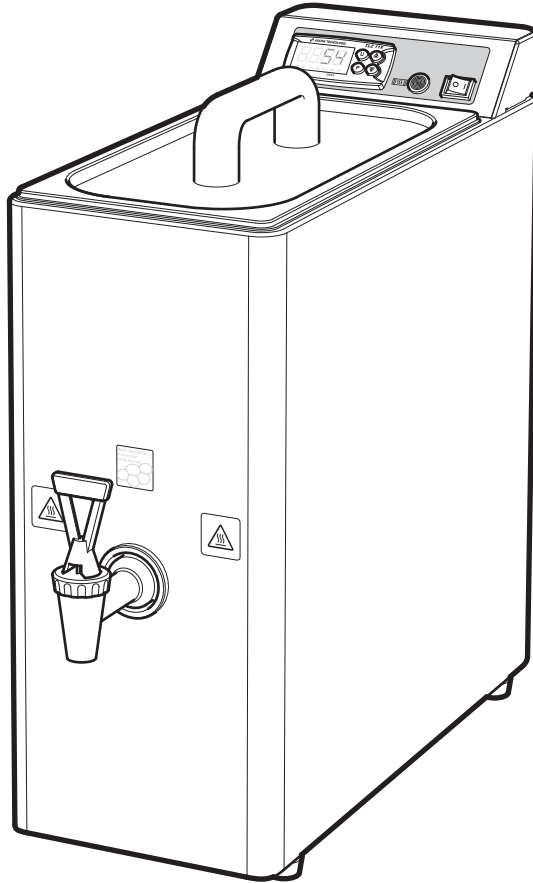


Instruction Manual
ET0003 Version 1.1

Cole-Parmer®
essentials

Introduction

Thank you for purchasing this Cole-Parmer product. To get the best performance from the equipment, and for your own safety, please read these instructions carefully before use.

Before discarding the packaging check that all parts are present and correct.

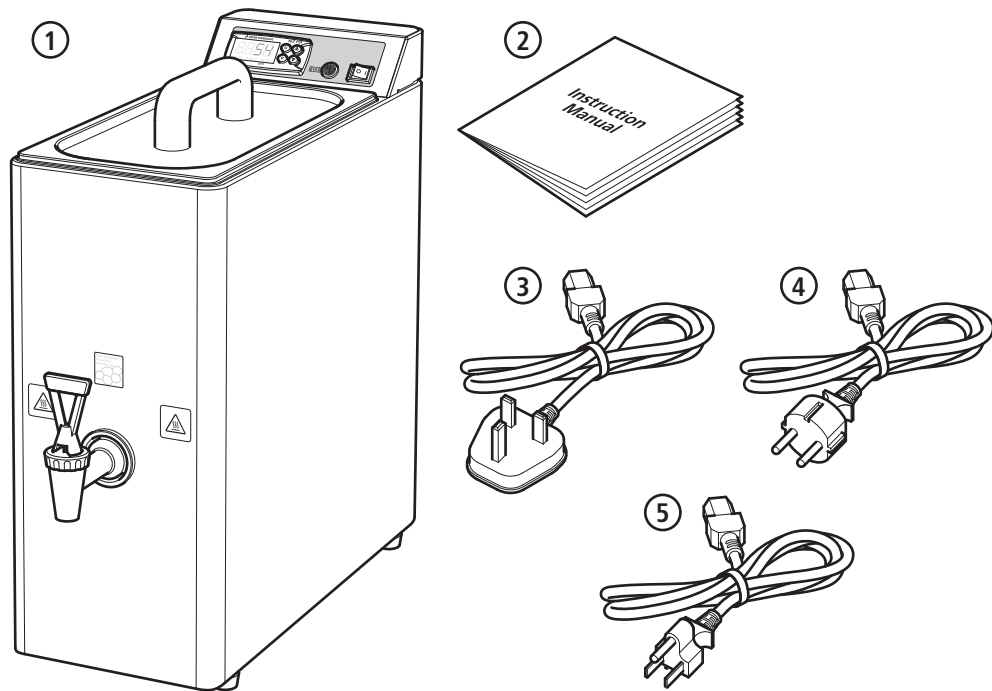

① Wax dispenser

② Instruction manual

③ UK power lead
(WD-200D only)

④ EU power lead
(WD-200D only)

⑤ US power lead
(WD-200D-120 only)

This equipment is designed to operate under the following conditions:

- ❖ For indoor use only
- ❖ Use in a well ventilated area
- ❖ Ambient temperature range 5°C to 40°C (41°F to 104°F)
- ❖ Altitude to 2000 m (6500 ft)
- ❖ Relative humidity not exceeding 80% (temperature 31°C) decreasing to 50% (temperature 40°C)
- ❖ Mains supply fluctuations not exceeding 10% of nominal
- ❖ Overvoltage category II IEC60364-4-443
- ❖ Pollution degree 2 IEC664
- ❖ Use with a minimum distance all round of 300 mm (12 in.) from walls or other items

If the equipment is not used in the manner described in this manual and with accessories other than those recommended by the manufacturer, the protection provided may be impaired.

General Description

The Wax Dispenser is designed for on-demand delivery of molten wax. The novel design of the instrument ensures that it takes up a minimum bench space in the laboratory, whilst still maintaining a large 7.5L capacity tank, for melting up to 6kg of pelletized wax at a time. The Wax Dispenser has digital temperature control which provides accurate temperature control of the molten wax, and is coupled with an ultra fast heating system for rapid melting of pelletized wax. Delivery of molten wax is via a non-drip lever tap, which is heated via a dedicated heating system, which prevents blockages resulting from solidified wax and ensures an even flow of wax. The inner tank has a filter screen (0.5mm mesh) fitted to prevent coarse particles from blocking the delivery tap. The tank is also fully insulated to prevent heat loss from the tank and to ensure that the outer surfaces of the tank are safe to touch.

Important Safety Advice

This product is designed for laboratory use only. Always follow good laboratory practice.

Users should be aware of the following safety advice:

- ❖ **DO NOT** use without appropriate training.
- ❖ **SHOCK HAZARDS OR UNSAFE PRACTICES ARE DANGEROUS** as they can cause severe personal injury, fire or death.
- ❖ **DO NOT** use combustible substances near hot objects.
- ❖ **DO NOT** use the equipment in hazardous atmospheres.
- ❖ **DO NOT** immerse the equipment in water.
- ❖ **DO NOT** operate or handle any part of the product with wet hands or use on surfaces that may become flooded.
- ❖ **NEVER** move the product while still connected to the power supply.
- ❖ **HIGH TEMPERATURES ARE DANGEROUS** as they can cause serious burns to operators and ignite combustible material.
- ❖ **USE CARE AND WEAR PROTECTIVE GLOVES TO PROTECT HANDS.**
- ❖ **NEVER** lift or carry the instrument during operation.
- ❖ **NEVER** use the tap to lift or carry the instrument.
- ❖ **DO NOT** position the unit so that it is difficult to disconnect from the mains supply using the mains plug.
- ❖ The mains outlet socket used should be located close to the equipment and readily identifiable and accessible to users.
- ❖ **DO NOT** leave equipment switched on and it is not recommended to leave any heating apparatus unattended during operation.
- ❖ The unit should be carried using both hands.
- ❖ **DO NOT** allow molten wax to accumulate on the surface of the equipment.
- ❖ **DO NOT** use if the equipment is empty
- ❖ **DO NOT** operate the tap while the wax is cold as this may damage the tap.

Symbols Defined



WARNING



HOT
SURFACE



RISK OF
ELECTRIC SHOCK



EARTH



BIOHAZARD

Electrical Requirements



THIS INSTRUMENT MUST BE GROUNDED

Before connection please ensure that the line supply corresponds to the power requirements below:

Power: 480W Supply requirements: 110 - 120 V or 220 - 240 V ~ 50/60Hz

The unit is provided with three power cables consisting of a UK 3-pin and a "Schuko" 2-pin plug for 230 V installations and a NEMA 5-15 plug for 120 V installations.

Choose the power cable appropriate for your electrical installation and discard the other. Should neither power cable be suitable for connecting to the power supply, replace the plug with a suitable alternative.

THIS OPERATION SHOULD ONLY BE UNDERTAKEN BY A QUALIFIED ELECTRICIAN.

NOTE: Refer to the equipment rating plate to ensure that the plug and fusing are suitable for the voltage and wattage stated. The wires in the mains cable are as follows:

230V

BROWN - HOT/LIVE

BLUE - NEUTRAL

GREEN/YELLOW – EARTH

120V

BLACK - HOT/LIVE

WHITE - NEUTRAL

GREEN - EARTH

The appropriate power cable and power adaptor combination should be connected to the instrument BEFORE connection to the mains supply. Should the mains lead require replacement, a heat resistant cable of 1.25mm² (AWG16) of harmonised code H05VV-F connected to an IEC320 plug should be used.



IF IN DOUBT CONSULT A QUALIFIED ELECTRICIAN



THIS EQUIPMENT MUST NOT BE FLASH TESTED

Safety Cut-outs

The equipment is protected by a miniature circuit breaker and a temperature cut out.

The miniature circuit breakers are located on the rear of the equipment. In the event of a fault, push back to reset. If the fault continues, please contact your local service representative or the service department of Antylia Scientific.

If the temperature cut-out is operated allow the equipment to cool completely. Identify and rectify the cause of cut-out operation before operating. If the temperature cut-out continues to operate, please contact your local service representative or the service department of Antylia Scientific.


Operation

Before Use

Place the unit on a firm, level surface, ensuring that all four feet on the base of the unit are positioned on the surface firmly. Avoid installation on a slippery surface or on a surface prone to vibration.


Note: Button **U** is not required in this application.

1. Ensure that the power cable is pushed fully into the power supply socket of the wax dispenser.
2. Connect the mains plug to the electrical supply.
3. Pour the desired quantity of wax into the internal tank. The tank has a maximum capacity of 7.5L which is large enough to melt 6.0kg of pelletized histology wax.
4. Turn ON the wax dispenser.
5. Set the desired temperature. Users are recommended to set the temperature 3-4°C above the melting point being used.

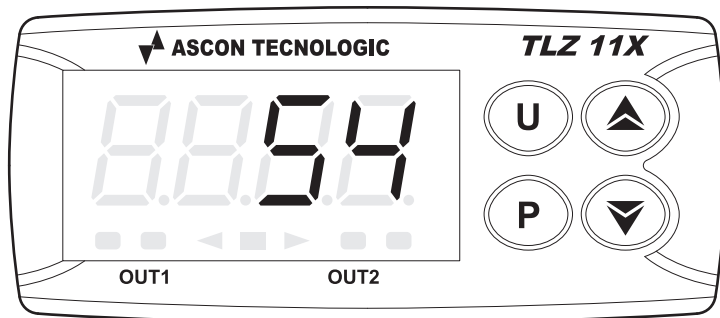


- a. Press **P** then release it (do not hold down **P** for more than 5 seconds).
- b. The display will show **SP** alternating with the current set temperature.
- c. To change the set temperature press **▲** to increase the value or **▼** to decrease it. These keys increase or decrease the value one digit at a time, but if the button is pressed for more than one second the value increases or decreases rapidly, and after two seconds pressed, the speed increases even more to allow the desired value to be reached rapidly.
- d. Exiting the Set mode is achieved by pressing **P** or automatically if no key is pressed for 15 seconds. After that time the display returns to the normal function mode.

6. The heater indicator will illuminate to show heater activity.
7. The equipment will warm up to the desired temperature and temperature rise will be shown on the display.
8. The wax dispenser is designed to melt bulk quantities of pelletized wax in as quick a time as possible. When set at 65°C the instrument will take roughly 90 minutes to fully melt 5kg of pelletized wax, with significant quantities of molten wax available for use after as little as 30 minutes.
9. Wax is delivered by pulling the tap lever forward. The tap has three positions:

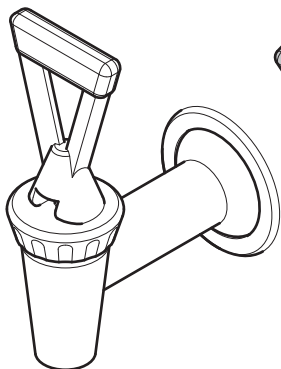

i Off

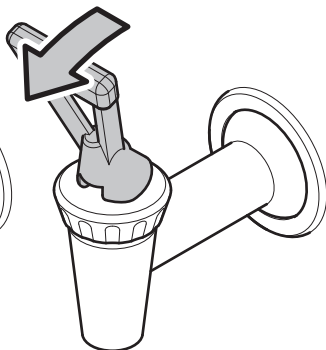

ii On demand pull dispense



iii Continuous flow - tap locked open



CAUTION: Do not operate the tap while the wax is cold as this may damage the tap.

Maintenance, Servicing and Cleaning



WARNING: Before attempting any maintenance, servicing or cleaning, ensure that the unit is cool.



WARNING: Do not touch any electrical contacts or open any closure plates.

RISK OF ELECTRIC SHOCK.



WARNING: Ensure the unit is disconnected from the power supply before attempting any maintenance, servicing or cleaning.

Regular cleaning of the instrument according to the cleaning instructions enclosed in this user manual will ensure that the instrument continues to operate efficiently and safely in normal everyday use. Cleaning or decontamination methods, other than those recommended in this guide, should be checked with your instrument supplier to ensure that the proposed method will not damage the instrument.

1. The outer case work of the Wax Dispenser, including the control panel, may be wiped using small quantities of mild detergent or polishes applied with a soft cloth.
2. The internal tank can be emptied by locking the delivery tap into the continuous flow position. Any residual wax at the bottom of the tank can be removed using absorbent tissues and wiped clean.
3. The filter (0.5mm mesh) situated at the bottom of the tank can be cleaned in-situ using a toothbrush or similar brush, or lifted out once the bolts are removed for more thorough cleaning using solvents. (If removing the filter it is recommended that protective gloves are worn).

NOTE: **DO NOT** use scouring pads, de-scaling agents or solvents to clean any parts of this equipment.

Preventative maintenance should include keeping the product clean by protecting it from spillage, contamination or corrosive environments. If in doubt, please confirm that any intended method of decontamination will not damage the equipment by contacting Antylia Scientific.

Antylia Scientific recommend that a simple annual inspection be made in order that any malfunction can be identified and rectified as early as possible. This is to ensure user safety and prolong instrument life span.

Recommended checks to be made:

1. Condition of Power Lead. A visual inspection to ensure the insulation is not damaged and that the correct fuse is fitted.
2. Functioning of Heater On Lamp. Heater lamp should be on when the instrument is warming up.
3. Condition of the wax dispenser tank and filter (0.5mm mesh). Both tank and filter should be in good condition with no evidence of corrosion and no damage visible to the filter screen.
4. Dispensing Tap Seal. The dispensing tap should seal correctly with no occurrence of constantly dripping wax when the tap is not in use.

NOTE: It is normal for a small quantity of molten wax to remain in the tap after it is closed. This residual wax will drip out, however it will be short lived and will be in very small quantities.

In Case of Contamination



WARNING: THE FOLLOWING PROCEDURE IS INTENDED AS A GUIDE. SHOULD SPILLAGE OF A TOXIC OR HAZARDOUS FLUID OCCUR, THEN ADDITIONAL SPECIAL PRECAUTIONS MAY BE NECESSARY.

If the equipment has been exposed to contamination, the Responsible Body is responsible for carrying out appropriate decontamination. If hazardous material has been spilt on or inside the equipment, decontamination should only be undertaken under the control of the Responsible Body with due recognition of possible hazards. Before using any cleaning or decontamination method, the Responsible Body should check with the manufacturer that the proposed method will not damage the equipment. Prior to further use, the Responsible Body shall check the electrical safety of the unit. Only if all safety requirements are met can the unit be used again.

NOTE: In the event of this equipment or any part of the unit becoming damaged or requiring service, the item(s) should be returned to the manufacturer for repair accompanied by a decontamination certificate. Copies of the Certificate are available from the Distributor/Manufacturer.

At the end of its service life, the product must be accompanied by a Decontamination Certificate.

Repairs and Support

Any repairs or replacement of parts **MUST** be undertaken by suitably qualified personnel. Only spare parts supplied or specified by Antylia Scientific or its agents should be used. Fitting of non-approved parts may affect the performance and safety features designed into the instrument. For a comprehensive list of parts required by service engineers conducting internal repairs please contact the service department quoting the model and serial number:

Email: cpSERVICE@antylia.com

Tel: +44 (0)1785 810475

For any other technical enquiries please contact the Technical Support Department at:

Email: cpTECHSUPPORT@antylia.com

Tel: +44 (0)1785 810433

Antylia Scientific Ltd,

Beacon Road,

Stone,

Staffordshire,

ST15 0SA,

United Kingdom

Email: cpSERVICE@antylia.com

Tel: +44 (0)1785 810475

Web: www.Cole-Parmer.com

Spares and Accessories

Please contact your local sales specialist or email cpSPARES@antylia.com to enquire about available spares.

Please visit www.Cole-Parmer.com for a full list of available accessories.

Technical Specification

General Specification



Safety functions	Class 1 cut out Thermal cut out 120°C
Tank cover	Stainless Steel
Tank material	Stainless Steel
Tank capacity	Approx. 7.5 litres
Maximum tank capacity	6kg
External dimensions	W181 x D499.5 (inc tap) x H455mm
Weight	7.0kg (without wax) 13.0kg (with Max. 6kg of wax)
Temperature display range	Ambient to 70°C (+/- 1°C at 20°C ambient)
Display resolution	1°C
Accuracy	± 1°C
Ceiling temperature setting	70°C
Display	Digital Display
Control Sensor	NTC Thermistor


Electrical specification

Total power consumption	480W
Total power output	5A
Temperature control	On/Off
Oven operating temperature range	Ambient to 70°C (+/- 1°C at 20°C ambient)
Electricity supply	110 - 120 V ~ 50/60Hz 220 - 240 V ~ 50/60Hz

Weights and Dimensions

Weight 7.0kg (without wax)
13.0kg (with Max. 6kg wax)

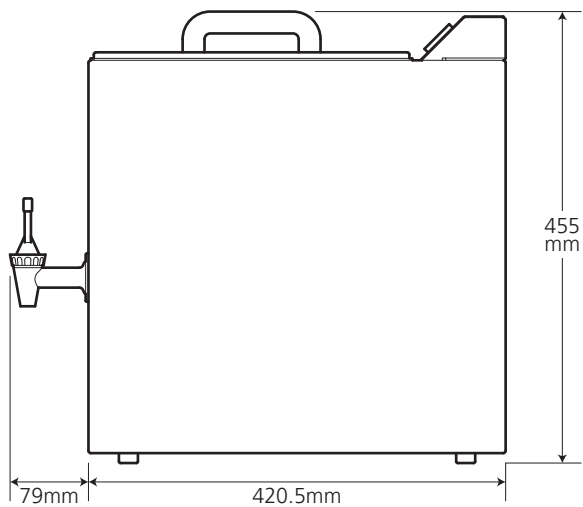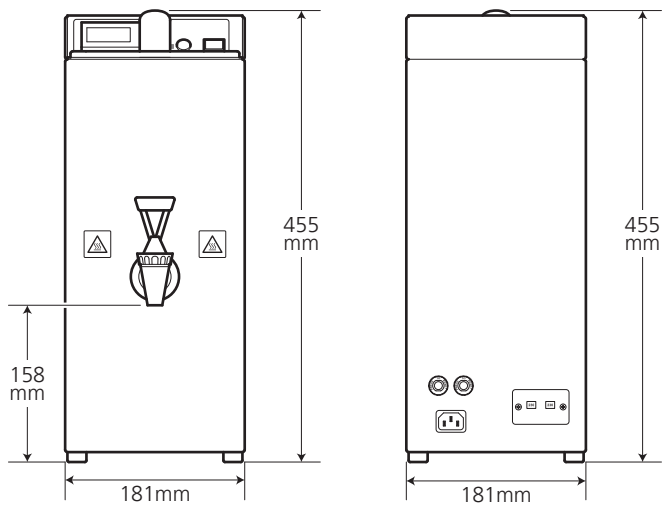

 This product meets the applicable CE Directives and UKCA Legislation for radio frequency interference and may be expected not to interfere with, or be affected by, other equipment with similar qualifications. We cannot be sure that other equipment used in its vicinity will meet these standards and so we cannot guarantee

that interference will not occur in practise. Where there is a possibility that injury, damage or loss might occur if equipment malfunctions due to radio frequency interference, or for general advise before use, contact the manufacturer.

Declaration of Conformity is available to view online at www.coleparmer.com

EU Representative address

Antylia Scientific GmbH
Futtererstraße 16
97877 Wertheim
Deutschland
Tel: +49 9377 9203-0
Email: sales@coleparmer.de

UK Representative address

Antylia Scientific
9 Orion Court
Ambuscade Road
Colmworth Business Park
St. Neots
PE19 8YX
United Kingdom
Tel: +44 (0) 1480 277339
Email: enquiries@antylia.com



WolfLabs

Pricing on any accessories shown can be found by keying the part number into the search box on our website.

The specifications listed in this brochure are subject to change by the manufacturer and therefore cannot be guaranteed to be correct. If there are aspects of the specification that must be guaranteed, please provide these to our sales team so that details can be confirmed.

www.wolflabs.co.uk

Tel : 01759 301142

Fax : 01759 301143

sales@wolflabs.co.uk

Please contact us if this literature doesn't answer all your questions.